

# CO<sub>2</sub> Incubator



**HCP-80E/168E/258E**

## Product Features

- Uniform and stable temperature
- Precise CO<sub>2</sub> concentration
- Quick environment recovery system in the incubator
- 90°C moist heat sterilization technology

**Qingdao Haier Biomedical Co.,Ltd.**

No.280 Feng Yuan Road, High-tech Zone,  
Qingdao, 266109, P.R. China  
E-mail: [inquiry@haierbiomedical.com](mailto:inquiry@haierbiomedical.com)  
Website: [www.haiermedical.com](http://www.haiermedical.com)



Haier Biomedical  
International



Haier Biomedical  
International



@haiermedicalint



Haier Biomedical  
International



Haier Biomedical  
International

## Product Parts



### Air Jacketed With Six-sides Heating Design

- Fast temperature recovery and superior temperature uniformity
- High temperature sterilization can ensure that the temperature of each surface can reach 90°C

### Door Switch

When the door opens, heating, air intake and fan automatically stop to minimize the risk of cross contamination

### Co<sub>2</sub> Sensor

- The new IR sensor with high temperature resistance of 100 °C, can withstand more than 300 high heat sterilization cycles
- Based on the NDIR measurement principle and uses a silicon MEMS transmitter to replace the traditional light source
- Zero drift and without need for calibration



### Partition

- Anti-slip design
- High levelness ensures uniform growth of adherent cells
- Mirror stainless steel to ensure high surface cleanliness, easy to clean



### Air Flow System

The air flow circulation ensures proper uniformity throughout the chamber

### Integrated Liner

Integral design, large arc design, easy to clean



### Inner Door

- Tempered glass provides easy observation of sample growth
- Three/six inner doors optional (HCP-168E)

### Operation Panel

- 4-inch LCD screen, vivid display and easy operation
- Abnormal operation sound and light alarm to ensure sample safety
- Running data can be traced, large capacity storage, data can be exported through USB



### Test Hole

Providing access for convenient measurement of internal statistics



### Outer Door


- Prevents the condensation of the inner door
- Left/right hand door optional

### Inner and Outer Door Seal

- Silicone material, prevent aging after heating
- Close the inner cavity to ensure the cleanliness and uniformity of the inner chamber

### Bottom Reservoir Humidification



- Reservoir humidification method, no water tray, easy to clean, avoid breeding bacteria
- Large evaporation area and fast humidity recovery

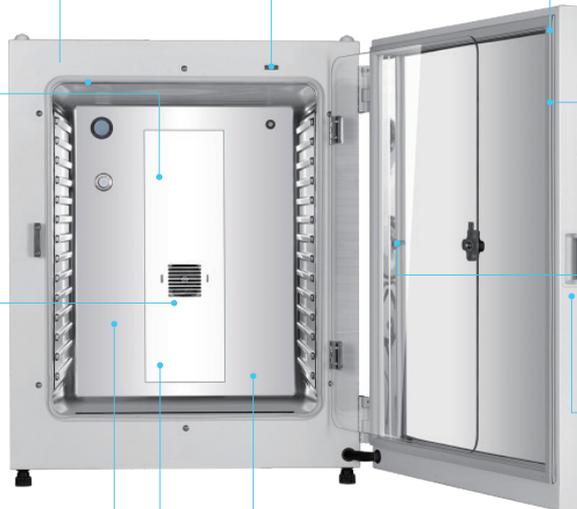


## Precise and Accurate Temperature Control



Controls the temperature precisely, within  $\pm 0.1^{\circ}\text{C}$ , with six-sided heating based on the fuzzy PID control principle, to provide a stable temperature to ensure the normal growth of cells throughout their life cycle.

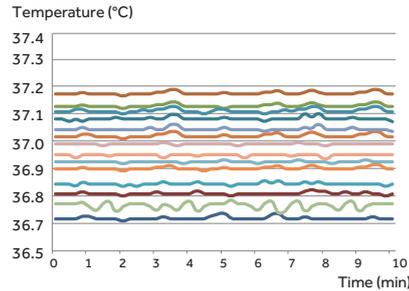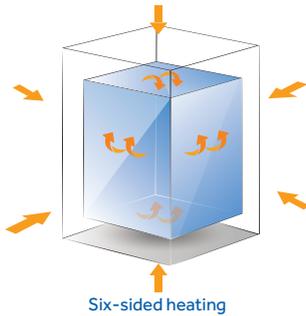

Uniformity of 27 measuring points  $\leq \pm 0.3^{\circ}\text{C}$

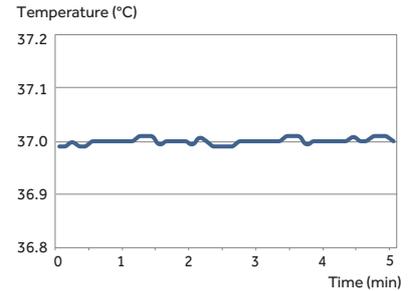


Central consistency point  $\leq \pm 0.1^{\circ}\text{C}$

## Precise CO<sub>2</sub> Concentration Using New IR Sensor Control Technology



### Precise CO<sub>2</sub> Concentration Using New IR Sensor Control Technology


Haier Biomedical's new IR Sensor technology uses NDIR measurement principles and withstands high temperature of  $100^{\circ}\text{C}$ . The silicon MEMS transmitter can carry out more than 300 dry heat sterilization cycles to extend the service life to 15 years. Built-in temperature and humidity compensation technology reduce the impact of changes in humidity and temperature without the need for calibration after the high temperature sterilization. Five points calibration yields a higher measuring accuracy, sensitivity with less drift (less than 0.3% within 2 years).

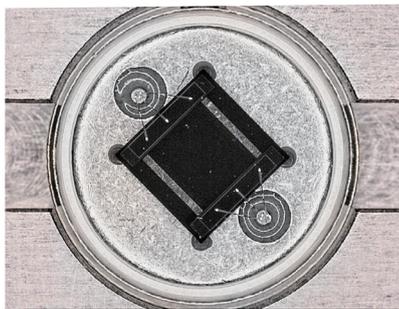

Silicon-based mems transmitter



Infrared (IR) sensor

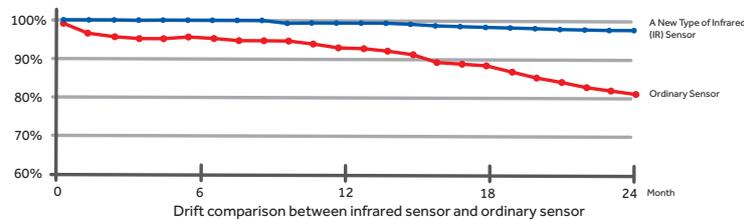

\*The equipment is tested by Haier in a controlled environment. Haier does not guarantee that the results of field tests under different conditions will be consistent. The test model is HCP-168E

## Fast Environment Recovery for Optimal Cell Growth



Adopting active air flow control technology, based on the fuzzy PID control principle, the parameters can be restored without overshoot. After opening the door for 30 seconds, the temperature and CO<sub>2</sub> concentration can be quickly restored within 4 minutes. Even if multiple users share a CO<sub>2</sub> incubator and frequently open and close the door, the stability and uniformity of the incubator can be ensured.






Illustration of purified airflow

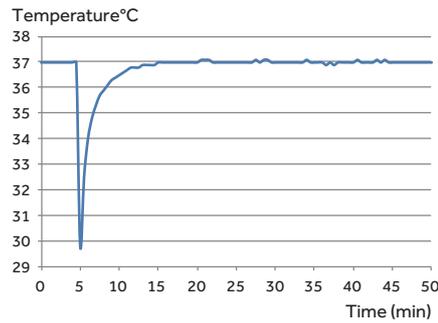

Temperature recovery curve (door open for 30s)

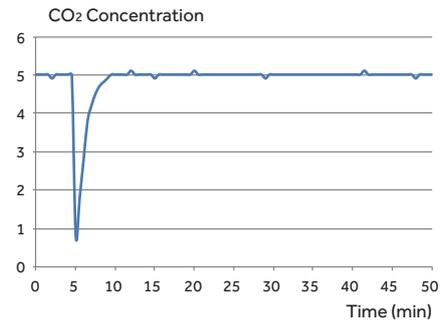

CO<sub>2</sub> concentration recovery curve (door open for 30s)


## 90°C Moist Heat Sterilization Technology



Effective sterilization of microorganisms including bacillus and spores with strong resistance, at 90°C under moist heat, without the need for consumables. Simply press the "sterilization button", to activate and complete the sterilization process automatically in 14 hours.

Delivers sterility level within the chamber of all surfaces to meet WS/T367-2012 standards.

All components are sterilized during the process, there is no need to disassemble internal components (including CO<sub>2</sub> sensors) and decontaminate separately, thus avoiding secondary pollution.

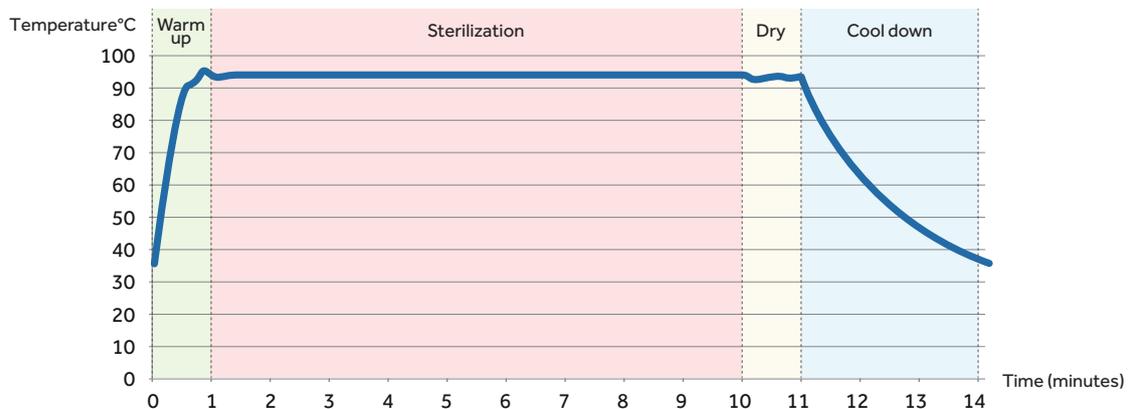

### Sterilization Temperature Profile


Forty-seven points were tested in the working chamber, including glass inner doors and partitions. All regions reached 90°C and maintained for 9 hours.

\*The equipment is tested by Haier in a controlled environment. Haier does not guarantee that the results of field tests under different conditions will be consistent. The test model is HCP-168E

## Easy to Clean Interior




The working chamber is plasma electro polished, stamped stainless steel with wide-arc, laser welded corners. Bracketless shelving design ensures that it is quick and easy to clean.

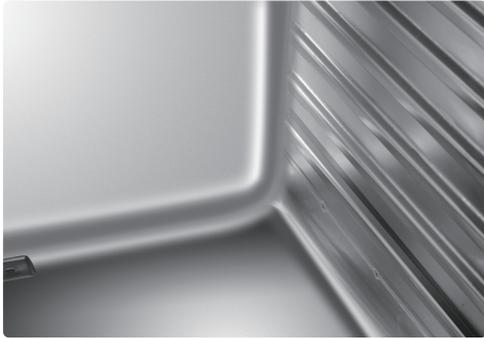

## Innovative Design with Attention to Detail



Safe anti-slip design of pull-out shelves.

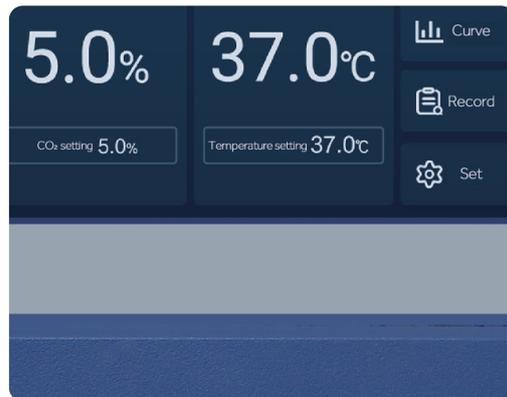

Data traceable for 15 years with large storage capacity and data exportable through USB.

## The Quality of ISO Class 5 Clean Room Can Ensure a Better Cell Growth Environment




The optional HEPA high-efficiency filtration system combined with the unique air duct circulation design can continuously filter pollutants (biological pollutants and suspended particles) in the cabinet, ensuring that the incubator can reach the ISO class 5 clean room within 5 minutes after the external door is closed, which is equivalent to the class 100 environment of the 209 E standard of the united states

## Reservoir Humidification Without Condensation



Active heat pipe condensation technology with condensate water directly returns to the reservoir, to ensure no condensation.

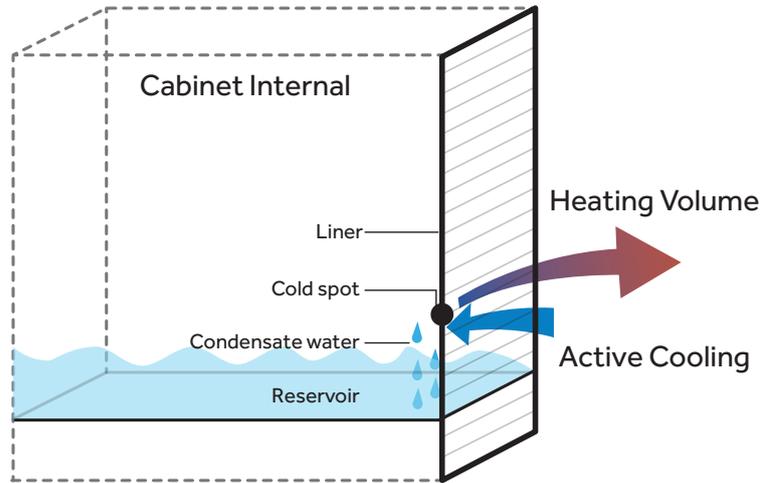

## Optional Accessories



Name	Material Description
Oxygen Module	Zirconia O <sub>2</sub> sensor, control accuracy: 0.1%; control range: 1-21% or 5-90%
3 Inner Door (for HCP-168E)	Reduce the temperature, humidity and carbon dioxide concentration in the box after opening the door, and minimize the mutual influence of multiple cultures
6 Inner Door (for HCP-168E)	Reduce the temperature, humidity and carbon dioxide concentration in the box after opening the door, and minimize the mutual influence of multiple cultures
8 Inner Door (for HCP-258E)	Reduce the temperature, humidity and carbon dioxide concentration in the box after opening the door, and minimize the mutual influence of multiple cultures
Water Tray	Provides different bottom humidification methods
Roller Base	Easy to move, prevent the ground bacteria contamination
HEPA Filter	Ensure the cleanliness of the cabinet, suitable for users who open and close the door frequently; After opening the door for 30 seconds, the air inside the cabinet can be passed through HEPA filters within 5 minutes and reach ISO 5 clean room quality
Pressure Reducing Valve	Suitable for users with cylinder gas supply
Shelf	Increase the number of samples cultured 4 materials : SUS304 single mirror surface SUS304 double mirror surface tempering glass Pure copper
Cylinder Switching	Supports switching between multiple steel cylinders to ensure uninterrupted air intake into the incubator
Stacking Bracket	Supports stacking of different volume models up and down, saving laboratory space
4-20mA	The analog acquisition interface for carbon dioxide and oxygen concentrations Multiple incubators can have the temperatures and carbon dioxide concentration data of all the incubators monitored at one computer terminal
Liner	SUS 304 SUS 316 Pure copper



Model		HCP-80E	HCP-168E	HCP-258E	
Type	Air Jacket				
Construction	Chamber Volume (L/Cu.Ft)	80/2.8	170/6.0	258/9.1	
	Interior Chamber	304 Stainless Steel			
	Exterior Chamber	Cold-Rolled Steel Powder Coated			
	Access Port	/	42mm Diameter	35mm Diameter	
Data Outputs	Remote Alarm Contacts, USB				
Dimensions	Net/Gross Weight (approx)	kg	75/90	95/125	110/150
		lbs	165/198	209.4/275	243/330
	Interior Dimensions (W*D*H)	mm	400*420*490	490*560*650	570*610*745
		in	15.7*16.5*19.3	19.3*22*25.6	22.4*24.0*29.3
	Exterior Dimensions (W*D*H)	mm	625*684*735	714*812*887	794*867*985
		in	24.6*26.9*28.5	28.1*32*34.9	31.3*34.1*38.8
Packing Dimensions (W*D*H)	mm	700*770*910	800*890*1050	870*950*1150	
	in	27.6*30.3*35.8	31.5*35.0*41.3	34.2*37.4*45.3	
Shelves	Dimensions (W*D)	mm	380*300	473*434	550*484
	Number Standard/Maximum	3/8			
	Max.Load Per Shelf/Total Load	kg	15/45		
	Construction	Perforated, Adjustable			
Electrical	Rated Voltage Power Supply (V/Hz)	220-240/50/60	220-240/50/60	220-240/50/60	
	Nominal Consumption (kw) (Steri-Run)	0.08 (1.0)	0.095 (1.5)	0.12 (1.8)	
Control	Controller	Microprocessor			
	Display	4 inch LED Button Screen			
CO <sub>2</sub>	Control Accuracy	0.10%			
	Range	0-20%			
	Alarm Range	±0.5%			
	Inlet Pressure	12-17PSI (0.8-1.2bar)			
	Gas Purity	Min.99.5% or Medical Quaiity			
	CO <sub>2</sub> Inlet	1/8" Hose (Barbed)			
	Senser	IR			
	Recovery Time ** (after 30s door opening .98% from initial value) Min	4			
CO <sub>2</sub> Inlet Filter (µm)	<0.2				
Alarms	High/Low Temperature	Y			
	Remote Alarm	Y			
	Sensor Error	Y			
	Excessive CO <sub>2</sub> Concentration	Y			
	Water Shortage Reminder	N			
	Door Ajar	Y			
Temperature Parameter	Control Accuracy (°C)	0.1			
	Range	Ambient Temperature+3-55°C			
	Uniformity	±0.3			
	Ambient Range (°C)	18-34			
	Temperature Fluctuations (°C)	±0.1			
	Senser	1*PT1000			
Recovery time *** (after 30s door opening .98% from initial value) Min	4				
Sterilization Cycle	Cycle Temperature	90°C Moist Heat Sterilization			
	Cycle Duration	Under 14 Hours			
Humidity	RH	93% ± 3% @ 37°C			
	Humidity Reservoir	Max.1.75L/Min 0.5L	Max.3.5L/Min 0.5L	Max.5.5L/Min 0.5L	
Option	HEPA Filter	Y	Y	Y	
	Pressure Reducing Valve	Y	Y	Y	
	4-20mA	Y	Y	Y	
	The Cylinder Switch	Y	Y	Y	
	Shelf	Y	Y	Y	
	Water Tray	Y	Y	Y	
	3 Inner Door	N	Y	N	
	6 Inner Door	N	Y	N	
	8 Inner Door	N	N	Y	
	Roller Base	Y	Y	Y	
	Pure Copper Inner Liner	Y	Y	Y	
	Pure Copper Shelf	Y	Y	Y	
	Humidity Display	N	N	N	
	Oxygen Module	Y	Y	Y	
	Electromagnetic Lock	N	N	N	
	Heightening Stand	Y	Y	Y	
IoT	Y	Y	Y		
Others	Certification	CE	CE	CE	

\*Product appearance and specifications are subject to change without notice

\*\* For CO<sub>2</sub> not exceeding 5.2%

\*\*\* For temperature not exceeding 37°C